











3M Filtek™ Z250

Universal Restorative System

Indications :
Class I, II, III, IV, V



Anterior Class III

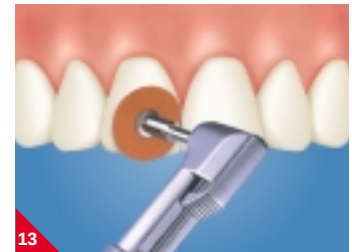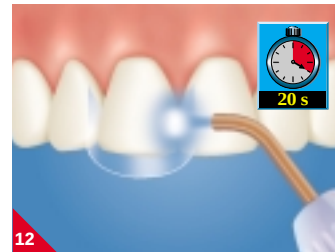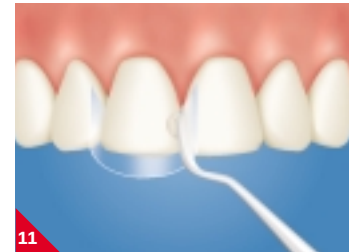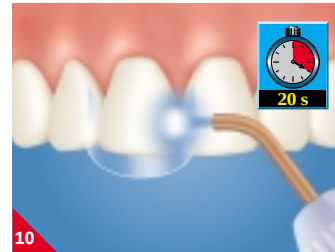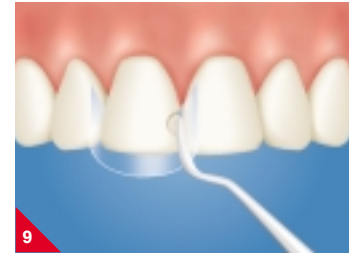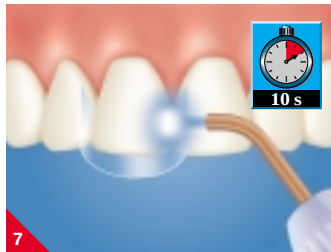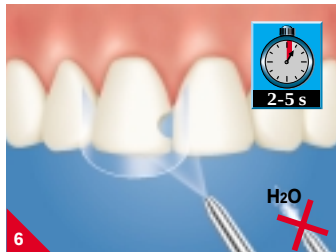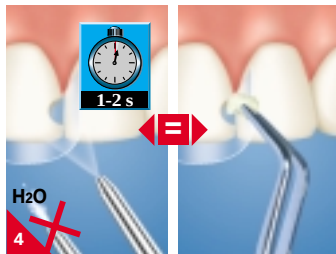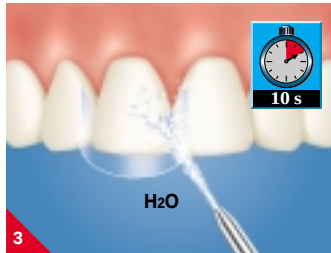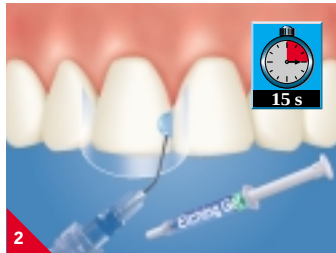

3M Filtek™ Z250

Universal Restorative System

Indications :
Class I, II, III, IV, V



Posterior Class II in molar




1



2




3

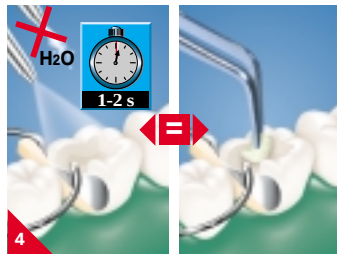

4



5

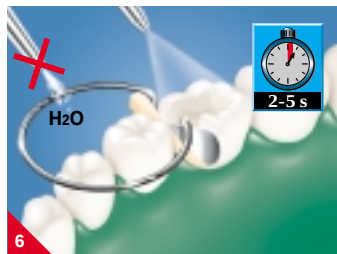

6



7




8



9



10

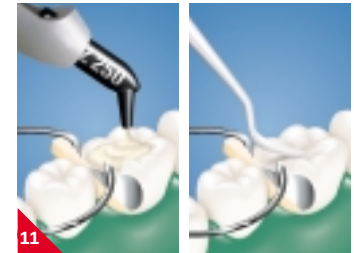

11



12



13